

Pressure gauges



Examples:



Model 213.40



Model 23x.50



Model 63x.50



Part of your business

Regulations for pressure equipment

- The pressure gauges are defined as "pressure accessories"
- The volume of the "pressure-bearing housings" of WIKA pressure gauges is < 0.1 L
- The pressure gauges carry conformity marking CE, UKCA for fluid group 1 per annex II, diagram 1 when their permissible working pressure is > 200 bar

Instruments that do not carry the mark are manufactured per article 4, paragraph 3 "sound engineering practice".

Applicable standards (depending on model)

- EN 837-1 Bourdon tube pressure gauges, dimensions, metrology, requirements and testing
- EN 837-2 Selection and installation recommendations for pressure gauges
- EN 837-3 Diaphragm and capsule pressure gauges, dimensions, metrology, requirements and testing

These operating instructions are only valid in conjunction with the data sheet of the respective instrument. The specifications given there must be observed.
See www.wika.com.

Subject to technical modifications.

© WIKA Alexander Wiegand SE & Co. KG 2009

Importer for UK
WIKA Instruments Ltd
Unit 6 and 7 Goya Business park
The Moor Road
Sevenoaks
Kent
TN14 5GY

WIKA Alexander Wiegand SE & Co. KG
Alexander-Wiegand-Straße 30
63911 Klingenberg/Germany
Tel. +49 9372 132-0
Fax +49 9372 132-406
info@wika.de
www.wika.de

2408976.08 10/2022

1. Safety



WARNING!

Before installation, commissioning and operation, ensure that the appropriate pressure gauge has been selected in terms of measuring range, design and suitable wetted material (corrosion) for the specific measuring conditions. In order to guarantee the measurement accuracy and long-term stability specified, the corresponding load limits must be observed.

The pressure measuring instruments may only be mounted by skilled personnel and after authorisation of the plant manager.

For hazardous media such as oxygen, acetylene, flammable or toxic gases or liquids, and refrigeration plants, compressors, etc., in addition to all standard regulations, the appropriate existing codes or regulations must also be followed.


From pressure gauges which do not correspond to a safety version per EN 837 highly pressurised media might leak out through the possibly bursting window in case of a component failure. For gaseous media and working pressures > 25 bar a pressure gauge with safety version S3 is recommended per EN 837-2.

After an external fire, pressure media can leak out, particularly at soft solder joints. All instruments must be checked and, if necessary, replaced before recommissioning the plant.

The safety instructions within these operating instructions, as well as the safety, accident prevention and environmental protection regulations for the application area must be maintained.

2. Mechanical connection

In accordance with the general technical regulations for pressure gauges (e.g. EN 837-2). When screwing the instruments in, the force required to do this must not be applied through the case, but only through the spanner flats provided for this purpose, and using a suitable tool.
For parallel threads, use flat gaskets, lens-type

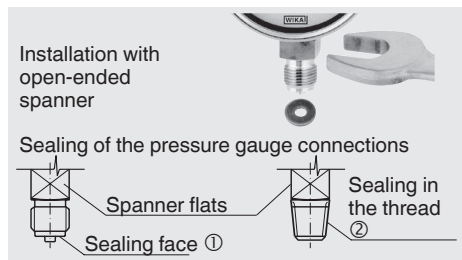

sealing rings or WIKA profile sealings at the sealing face ①. With tapered threads (e.g. NPT threads), sealing is made in the threads ② using additional sealing materials, e.g. PTFE tape.

The torque depends on the sealing used. In order to orientate the measuring instrument so that it can be read as well as possible, a connection with clamp socket or union nut should be used.

When a blow-out device is fitted to a pressure gauge, it must be protected against being blocked by debris and dirt. With safety pressure gauges (see ⑤) there must be a free space of > 20 mm behind the blow-out back.



After installation, open the vent valve (if present) or set from CLOSE to OPEN. The version of the vent valve depends on the model and can deviate from the above illustration!

Requirements for the installation point

If the line to the measuring instrument is not adequately stable, a measuring instrument holder should be used for fastening (and possibly via a flexible capillary). If vibrations cannot be avoided by means of suitable installation, instruments with liquid filling should be used. The instruments should be protected against coarse dirt and wide fluctuations in ambient temperature.

3. Permissible ambient and operating temperatures

When mounting the pressure gauge it must be ensured that, taking into consideration the influence of convection and heat radiation, no deviation above or below the permissible temperature limits can occur. Observe the influence of temperature on the indication accuracy!

4. Storage

To protect the pressure gauges from mechanical damage keep them in the original packaging until installation.
Protect the measuring instruments from humidity and dust.

Storage temperature range: -40 ... +70 °C

Storage temperature range model

PG23LT: -70 ... +70 °C

5. Maintenance and repairs

The pressure gauges are maintenance-free. Regular checks should be carried out to ensure the measurement accuracy.

In the case of pressure measuring instruments with blow-out devices or safety pressure gauges, the safety elements (e.g. blow-out plug or blow-out back) must be replaced after 10 years. The replacement may only be carried out by skilled personnel using original parts and after authorisation of the plant manager.

When dismantling, close the vent valve (if present).



WARNING! Residual media in dismantled pressure gauges can result in a risk to persons, the environment and equipment. Take sufficient precautionary measures.